



RoHS III
COMPLIANT

UK
CA

EAC




Operation manual

DA03 GK/HLP (ATEX)

Differential pressure measuring device
Pressure levels PN40/PN100/PN160

Models for use in
explosive areas

DA03 ... 0A
DA03 ... 1B
DA03 ... 1C
DA03 ... 2D



Masthead

Manufacturer:**FISCHER Mess- und Regeltechnik GmbH**

Bielefelderstr. 37a
D-32107 Bad Salzuflen

Telephone: +49 5222 974 0
Telefax: +49 5222 7170

eMail: info@fischermesstechnik.de
web: www.fischermesstechnik.de

Technical editorial team:

Technical editor: R. Kleemann

All rights, also those to the translation, reserved. No part of this document may be reproduced or processed, duplicated or distributed using electronic systems or any other form (print, photocopy, microfilm or another process) without the written consent of the company FISCHER Mess- und Regeltechnik GmbH, Bad Salzuflen.

Reproduction for internal use is expressly allowed.

Brand names and procedures are used for information purposes only and do not take the respective patent situation into account. Great care was taken when compiling the texts and illustrations. nevertheless, errors cannot be ruled out. The company FISCHER Mess- und Regeltechnik GmbH will not accept any legal responsibility or liability for this.

Subject to technical amendments.



© FISCHER Mess- und Regeltechnik 2018

Version history

Rev. ST4-A 09/17	Version 1 (first edition)
Rev. ST4-B 09/19	Version 2 (accessories updated)
Rev. ST4-C 10/21	Version 3 (UKCA Declaration)
Rev. ST4-D 02/23	Version 4 (liquid filling for inductive contacts)
Rev. ST4-E 07/23	Version 5 (model T omitted)
Rev. ST4-F 02/24	Version 6 (measuring cell Ø75 pressure caps changed)
Rev. ST4-G 02/25	Version 7 (0...600 mbar measuring range not applicable for 130 measuring cell, ATEX update)

Table of Content

1 Safety guidelines.....	4
1.1 General.....	4
1.2 Personnel Qualification	4
1.3 Risks due to Non-Observance of Safety Instructions	4
1.4 Safety Instructions for the Operating Company and the Operator	4
1.5 Unauthorised Modification	5
1.6 Inadmissible Modes of Operation	5
1.7 Safe working practices for maintenance and installation work	5
1.8 Pictogram explanation	6
2 Product and functional description.....	7
2.1 Delivery scope	7
2.2 Equipment versions	7
2.3 Intended use.....	11
2.4 Function diagram.....	11
2.5 Design and mode of operation	12
3 Assembly	13
3.1 General information	13
3.2 Process connection	13
3.3 Electrical connections.....	14
3.4 Use in areas at risk of explosion	17
4 Commissioning	21
4.1 General.....	21
4.2 Venting of the pressure lines	21
4.3 Zero point correction	22
4.4 Switch point setting	22
5 Servicing	24
5.1 Maintenance	24
5.2 Maintenance	24
5.3 Transport	24
5.4 Service	24
5.5 Disposal.....	25
6 Technical data	26
6.1 General information	26
6.2 Input variables	27
6.3 Operating conditions	28
6.4 Construction design.....	28
7 Order Codes	35
7.1 Accessories	38
8 EU Declaration of Conformity	39
9 UKCA Declarations of Conformity.....	44
10EAC Declaration	52

1 Safety guidelines

1.1 General

This operating manual contains basic instructions for the installation, operation and maintenance of the device that must be followed without fail. It must be read by the installer, the operator and the responsible specialist personnel before installing and commissioning the device.

This operating manual is an integral part of the product and therefore needs to be kept close to the instrument in a place that is accessible at all times to the responsible personnel.

The following sections, in particular instructions about the assembly, commissioning and maintenance, contain important information, non-observance of which could pose a threat to humans, animals, the environment and property.

The instrument described in these operating instructions is designed and manufactured in line with the state of the art and good engineering practice.

1.2 Personnel Qualification

The instrument may only be installed and commissioned by specialized personnel familiar with the installation, commissioning and operation of this product.

Specialized personnel are persons who can assess the work they have been assigned and recognize potential dangers by virtue of their specialized training, their skills and experience and their knowledge of the pertinent standards.

For explosion-proof models the specialized personnel must have received special training or instruction or be authorized to work with explosion-proof instruments in explosion hazard areas.

1.3 Risks due to Non-Observance of Safety Instructions

Non-observance of these safety instructions, the intended use of the device or the limit values given in the technical specifications can be hazardous or cause harm to persons, the environment or the plant itself.

The supplier of the equipment will not be liable for damage claims if this should happen.

1.4 Safety Instructions for the Operating Company and the Operator

The safety instructions governing correct operation of the instrument must be observed. The operating company must make them available to the installation, maintenance, inspection and operating personnel.

Dangers arising from electrical components, energy discharged by the medium, escaping medium and incorrect installation of the device must be eliminated. See the information in the applicable national and international regulations.

Please observe the information about certification and approvals in the Technical Data section.

The instrument must be decommissioned and secured against inadvertent re-operation if a situation arises in which it must be assumed that safe operation is no longer possible. Reasons for this assumption could be:

- evident damage to the instrument
- failure of the electrical circuits
- longer storage outside the approved temperature range.
- considerable strain due to transport

Repairs may be carried out by the manufacturer only.

A professional single conformity inspection as per DIN EN 61010, section 1, must be carried out before the instrument can be re-commissioned. This inspection must be performed at the manufacturer's location. Correct transport and storage of the instrument are required.

1.5 Unauthorised Modification

Modifications of or other technical alterations to the instrument by the customer are not permitted. This also applies to replacement parts. Only the manufacturer is authorised to make any modifications or changes.

1.6 Inadmissible Modes of Operation

The operational safety of this instrument can only be guaranteed if it is used as intended. The instrument model must be suitable for the medium used in the system. The limit values given in the technical data may not be exceeded.

The manufacturer is not liable for damage resulting from improper or incorrect use.

1.7 Safe working practices for maintenance and installation work

The safety instructions given in this operating manual, any nationally applicable regulations on accident prevention and any of the operating company's internal work, operating and safety guidelines must be observed.

The operating company is responsible for ensuring that all required maintenance, inspection and installation work is carried out by qualified specialized personnel.

1.8 Pictogram explanation



DANGER

Type and source of danger

This indicates a **direct** dangerous situation that could lead to death or **serious injury** (highest danger level).

1. Avoid danger by observing the valid safety regulations.



WARNING

Type and source of danger

This indicates a **potentially** dangerous situation that could lead to death or **serious injury** (medium danger level).

1. Avoid danger by observing the valid safety regulations.



CAUTION

Type and source of danger

This indicates a **potentially** dangerous situation that could lead to slight or serious injury, damage or **environmental pollution** (low danger level).

1. Avoid danger by observing the valid safety regulations.



NOTICE

Note / advice

This indicates useful information of advice for efficient and smooth operation.

2 Product and functional description

2.1 Delivery scope

- Differential pressure measuring device DA03
- Operating Manual

2.2 Equipment versions

The following illustrations depict typical combinations of the measuring cell, measured value display and contact elements. However, these can be freely combined according to the order code. Wherever this is not possible, this is clearly stated.

For instance, a small measuring cell with an NG160 display and a contact element is also available.

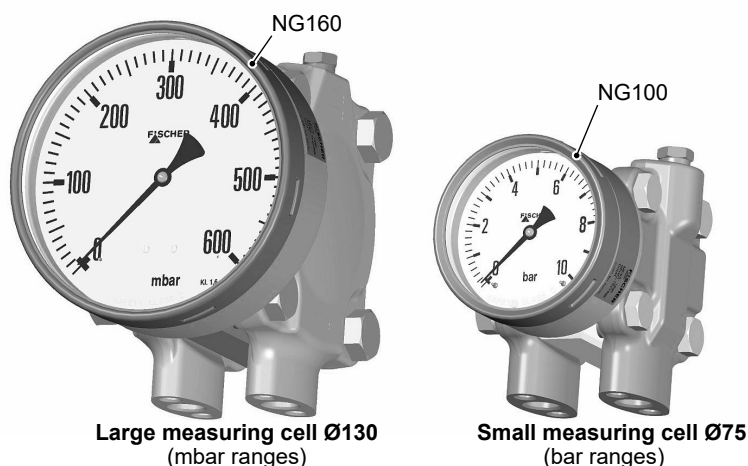


Fig. 1: Device overview

2.2.1 Process connection

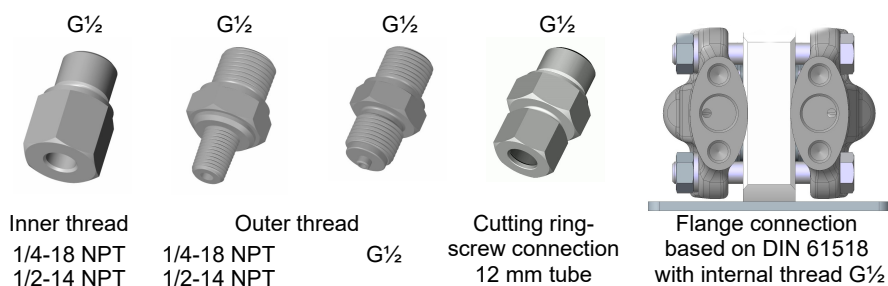
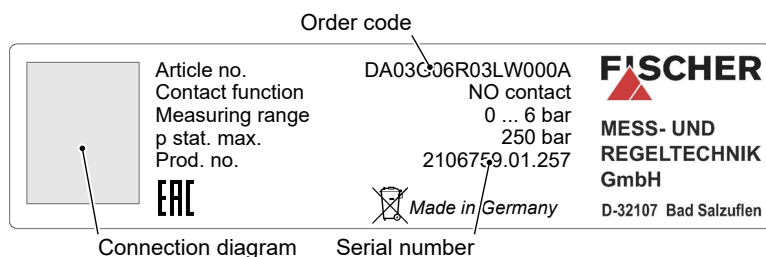


Fig. 2: Options for the process connection

2.2.2 Nameplate

The presented type plates serve to show an example of the information shown. The data shown is purely fictive, but does correspond to the actual conditions. For more information, please see the order code at the end of these instructions.




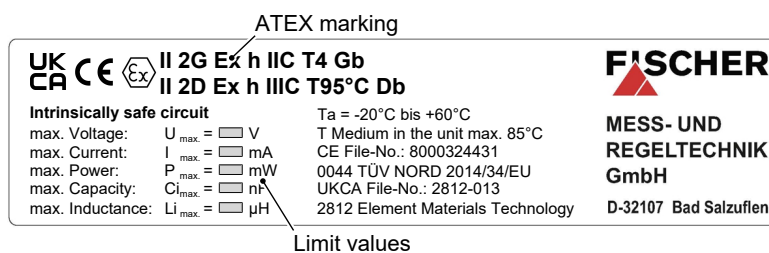


Fig. 3: Nameplate

2.2.3 Contact elements

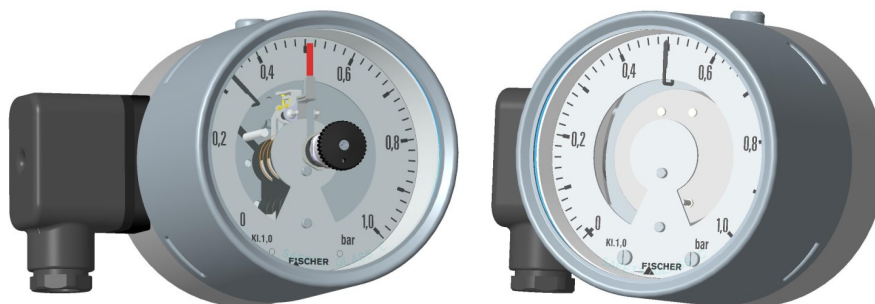

Limit switch in accordance with data sheet KE##	Rotation angle encoder in accordance with data sheet KE09
for standard devices	
<ul style="list-style-type: none"> • Low-action contacts • Snap-actiocontacts • Inductive contacts 	<ul style="list-style-type: none"> • KINAX 3W2 708-226D0 • KINAX 3W2 708-226E0
for ATEX devices	
<ul style="list-style-type: none"> • Snap-action contacts • Inductive contacts 	<ul style="list-style-type: none"> • KINAX 3W2 708-226D0 • KINAX 3W2 708-226E0

Fig. 4: Contact elements

2.2.4 Special functions



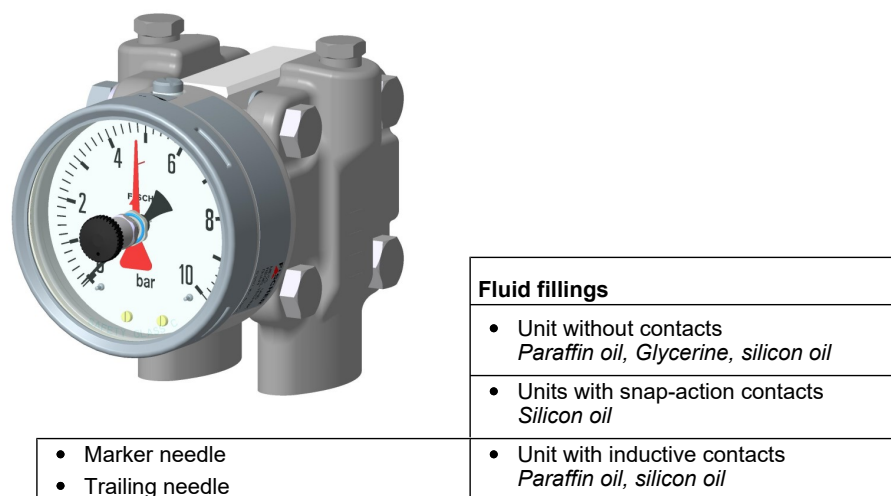


Fig. 5: Special functions


2.2.5 Assembly

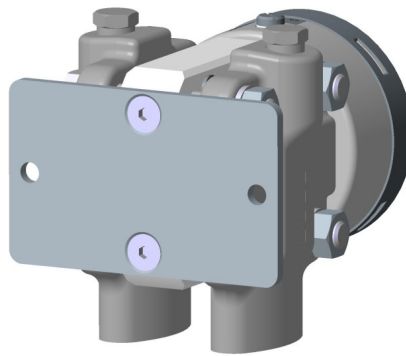

Wall mounting

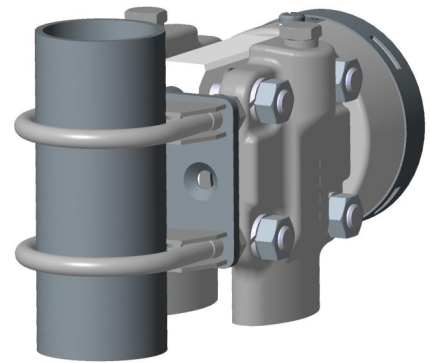

Pipe mounting

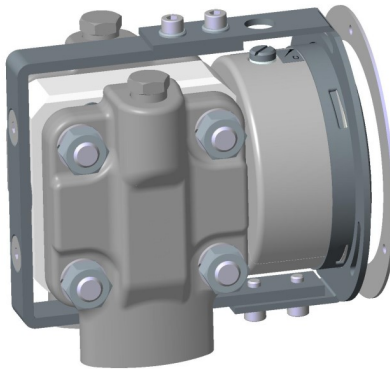

Panel mounting set type 1
with panel mounting set



Panel mounting set type 2
with front ring

Fig. 6: Assembly types

The panel installation fittings can only be used in devices with a small measuring cell ($\varnothing 75$) and a display in the NG100 bayonet ring casing.



WARNING

Panel mounting set

Due to the heavy weight, the operator needs to install a support construction for installation of the front panel.

2.2.6 Equipment features (overview)

The following shows the configuration possibilities of the DA03 depending on the measuring cell used and the pressure level.

NOTICE! All PN160 versions are only possible with one switching contact.

Key

- available for PN40/PN100/PN160
- only available for PN40/PN100
- on request

Small measuring cell Ø75

Measurement range	Measurement display		Low-action contacts			Snap-action contacts			Inductive contacts		Rot. angle transducer	Trailing needle	Marker needle	Remote seal	Pressure level
	Ø100	Ø160	1	2	3	1	2	3	1	2					
0 ... 0.6 bar	○	○				○	○		○	○	○	○	○	○	PN40/PN100
0 ... 1 bar	○	○				○	○		○	○	○	○	○	○	
0 ... 1.6 bar	○	○				○	○		○	○	○	○	○	○	
0 ... 2.5 bar	○	○				○	○		○	○	○	○	○	○	
0 ... 4.0 bar	○	○				○	○		○	○	○	○	○	○	
0 ... 6bar	○	○				○	○		○	○	○	○	○	○	
0 ... 10 bar	○	○				○	○		○	○	○	○	○	○	
0 ... 16 bar	○	○				○	○		○	○	○	○	○	○	
0 ... 25 bar	○	○				○	○		○	○	○	○	○	○	
-1 ... 0.6 bar	○	○				○	○		○	○	○	○	○	○	
-1 ... 1.5 bar	○	○				○	○		○	○	○	○	○	○	
-1 ... 3 bar	○	○				○	○		○	○	○	○	○	○	
-1 ... 5 bar	○	○				○	○		○	○	○	○	○	○	

Large measuring cell Ø130

Measurement range	Measurement display		Low-action contacts			Snap-action contacts			Inductive contacts		Rot. angle transducer	Trailing needle	Marker needle	Remote seal	Pressure level
	Ø100	Ø160	1	2	3	1	2	3	1	2					
0 ... 40 mbar	○	○				□	□		□	□	○		○		PN40 PN100
0 ... 60 mbar	○	○				○	○		○	○	○	○	○		
0 ... 100 mbar	●	●				●	○		●	○	●	●	●	●	PN40/PN100/PN160
0 ... 160 mbar	●	●				●	○		●	○	●	●	●	●	
0 ... 250 mbar	●	●				●	○		●	○	●	●	●	●	
0 ... 400 mbar	●	●				●	○		●	○	●	●	●	●	
-40 ... +60 mbar	●	●				●	○		●	○	●	●	●	●	
-60 ... +100 mbar	●	●				●	○		●	○	●	●	●	●	
-100 ... +150 mbar	●	●				●	○		●	○	●	●	●	●	
-100 ... +250 mbar	●	●				●	○		●	○	●	●	●	●	

2.3 Intended use

The DA03 serves to display differential pressures in neutral gaseous and fluid media.

If used with aggressive media, the media compatibility with the materials used must be checked (see Techn. data).

The DA03 can be delivered with a contact element. If the set limit values are exceeded, the output power circuits are opened or closed, and/or a 0/4...20 mA output signal proportional to the displayed value is issued for a capacitive rotation angle encoder.



DANGER

Installation regulations

The respective installation instructions must be observed for every application case. These should be listed in detail in the same-named section in chapter 'Assembly' for the 'use in explosive areas'.

2.4 Function diagram

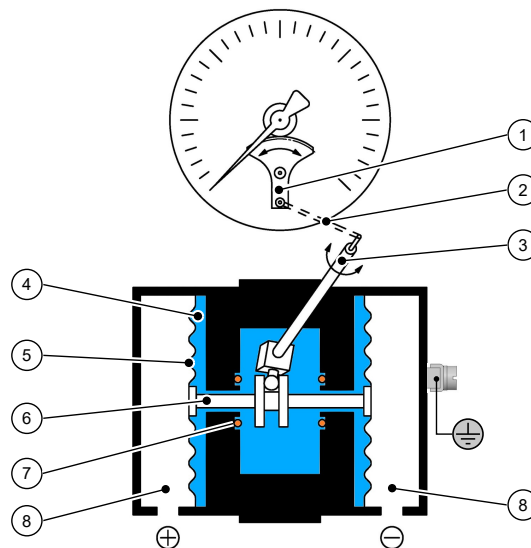


Fig. 7: Function diagram

1	Motion train	2	Transfer lever
3	Measuring shaft	4	Pressure transfer fluid
5	Measuring membranes	6	Connecting rod
7	O-ring (pressure relief valve)	8	Pressure chamber

2.5 Design and mode of operation

The pressures in the pressure chambers that are to be compared are each exerted onto a measuring membrane that can be rigidly connected using a connection rod. To compensate the static pressure, the space between the measuring membranes is filled with a pressure transfer fluid.

During pressure equalisation, the two measuring membranes are in an idle position. In case of pressure difference, the force acting on the membranes causes it to be moved towards the side of the lower pressure.

The connecting rod transfers the deflection of the measuring membranes onto the transfer lever mounted to the measuring shaft. Proportional to the current differential pressure, the measurement shaft makes a rotational movement that the indicator translates into a rotation angle between 0 and 270°.

In the case of one-sided pressure by the measuring system above and beyond the measuring range, the over-pressure guard will be activated. The over-pressure causes the overloaded membrane and its collar to be pressed against the inner O-ring. This creates two separate pressure spaces between the measuring membranes that need to be filled with fluid. In the adjacent pressure space, a corresponding over-pressure is created. The measuring membrane is supported by the contained transfer fluid. In this way the measuring membranes compensate the forces acting upon them.

3 Assembly

3.1 General information

The device can be mounted in one of the following ways (see Assembly [► 9]):

1. Wall mounting

The device is designed for installation onto flat assembly plates. The unit is equipped with a wall mounting plate for this mounting type.

2. Pipe assembly

The device is equipped with a special pipe assembly set and is suitable for mounting to a 2" pipe (DN50).

3. Panel mounting

Panel mounting is available in two installation models.

– Panel mounting fittings (Type 1)

This variant is only suitable for models with a small measuring system (Ø75) and a bayonet ring casing NG100.

– Panel installation with front ring (Type 2)

All models are suitable for this variant. A suitable steel construction must be used to ensure that the front plate can bear the weight of the DA03. This is possible e.g. by means of a combination with the wall or pipe assembly.

At the factory, the device is calibrated for vertical installation, but the installation position is arbitrary. For any installation positions that are not vertical, the zero-point signal can be corrected via the installed offset correction.

To ensure safety during installation and maintenance, we recommend installing a suitable shut-off valve on the system (see accessories).

3.2 Process connection

- By authorized and qualified specialized personnel only.
- The pipes need to be depressurized when the instrument is being connected.
- Appropriate steps must be taken to protect the device from pressure surges.
- Check that the device is suitable for the medium being measured.
- Maximum pressures must be observed (cf. Tech. data)

All supply lines are arranged so that there are no mechanical forces acting on the device.

The pressure lines must be kept as short as possible and installed without any tight bends to avoid delays.

The pressure lines must be installed at an inclination so that when fluids are measured no air pockets are created or when measuring gases, no water pockets are created. If the required inclination is not reached, water or air filters must be installed at suitable places.

With liquid measuring media, the pressure lines must be vented [► 21].

If water is used as a measuring medium, the unit must be protected against frost.

If the pressure sensing lines are already pressurised at the time of commissioning, zero-point control and adjustment cannot be performed. In such cases, the device should be only connected to the mains without the pressure sensing lines.

The process connections are marked on the unit with (+) and (-) symbols. The pressure lines are to be mounted according to this marking.

Differential pressure

- ⊕ Higher pressure
- ⊖ lower pressure




Fig. 8: Process connection

3.3 Electrical connections



⚠ DANGER

Operation in areas at risk of explosion

If operated in explosive areas, the electrical data of the unit and the valid local regulations and guidelines for the installation and operation of electrical systems in explosive areas must be observed.

- The electrical connection may only be completed by authorised and qualified specialists that have undergone additional training or briefings or have a permit to work on explosion-protected units in potentially explosive systems.
- Risks emanating from electrical current or voltage should be prevented by means of suitable measures.
- When the device is connected, national and international electrotechnical regulations must be observed.
- Disconnect the system from the mains before electrically connecting the device.
- Do not connect the connector if strained.
- Install the consumption-appropriate fuses.

Only devices with contact elements are connected to the electrical supply. To this end there is a cable socket on the side of the device, or a HAN plug in the power plant model.

The outer ground connection must always be connected to the protective potential equalisation or a similar local potential equalisation. The connection is suitable for connecting fine-wire conductors up to 4 mm² or single-wire conductors up to 6 mm².

The installed cables and wires must be tested with a reduced tensile force (25%) in compliance with Section A.3.1 of the standard EN 60079-0 and may only be used for permanent installation of operating equipment of Group II. The operator must ensure that the cables are connected with clamps accordingly.

The following data applies to the cable gland:

Cable gland	M20 x 1.5
Cable diameter	7 ... 13 mm
Max. conductor cross-section	1.5 mm ²
Tightening torque	3 Nm (clockwise tight)
Key width	21

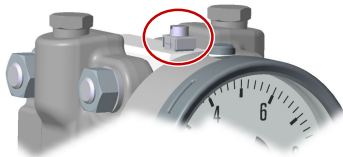


Fig. 9: Earthing connection

3.3.1 Cable socket (blue)

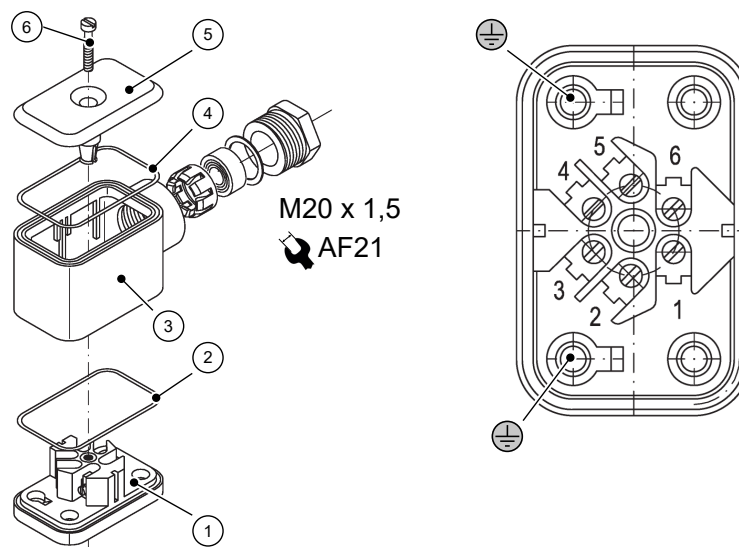


Fig. 10: Cable socket

1	Lower part	2	Sealing ring EPDM
3	Middle part	4	Sealing ring EPDM
5	Cover	6	Lid screw

3.3.2 Contact elements

Contact elements are supplied in accordance with data sheet KE. This illustrates all variants, their pin assignment and the technical data.

Magnetic spring contacts

The terminal numbers always correspond to the contact number and are assigned to the target indicators from left to right. Up to three contacts can be used. There are assigned to the target indicators as follows:

Contact 1: left target indicator
Contact 2: right target indicator.




Fig. 11: Contacts

Inductive contacts

In the case of inductive contacts, the switch function is not only determined by the slot type initiator but also by the switch amplifier. Up to max two contacts can be used. There are assigned to the target indicators as follows:

Contact 1: left target indicator
Contact 2: right target indicator.





Fig. 12: Inductive contacts

3.3.3 Rotation angle transducers KINAX 3W2

The rotation angle encoder serves to record angular positions, to prepare and provide the measured values as electrical output signals 0/4 ... 20 mA for the following device. Rotation angle encoder is supplied in accordance with data sheet KE09. This contains further information about the pin assignment and the technical data.

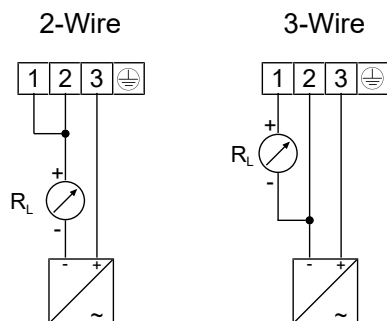

$$E_b = 12 \dots 30V$$

Fig. 13: Rotation angle transducers connection

3.4 Use in areas at risk of explosion

3.4.1 Differential pressure transmitter without contact element

DA03 ... 0A

Ex II 2G Ex h IIC T4 Gb

Ex II 2D Ex h IIC T95°C Db

Explosive areas Zone 1 and 2, and 21 and 22, risk from gases and dry dust.

Allowed temperatures:

- The maximum surface temperature 95 °C was determined under the following conditions without dust accumulation and safety factor.
- Allowed ambient temperature: -20°C to +60°C.
- Allowed medium temperature in the differential measurement unit < 85°C.



WARNING

Compression heat

With gaseous mediums, the instrument temperature can increase due to compression heat. In such cases, the pressure change speed must be limited or reduced to the allow measuring substance temperature.

NOTICE! For a differential pressure change between 10% and 90% of the measuring range and a pulse frequency < 0.06 Hz, the temperature increase is <10K.

To avoid additional heating, the instruments may not be exposed to direct sunlight during operation.

The standards EN60079-0, EN 60079-31, EN ISO 80079-36 and EN ISO 80079-37 apply for the non-electrical part of the devices in terms of explosion protection. The applicable requirements of these standards are satisfied.

(a) European market (CE):

The documentation for the mechanical part were filed with the notified body NB 0044 TÜV-Nord-Cert under file number 8000324431.

(b) UK market (UKCA):

The documentation for the mechanical part were filed with the notified body NB 2812 Element Material Technology under file number 2812-013.

(c) Eurasian Economic Union (EAC):

The unit does not have ATEX approval for this market. It may only be used there as an industrial unit.

3.4.2 Differential pressure transmitter with magnetic spring contacts

DA03 ... 1B

II 2G Ex h IIC T4 Gb

Simple electric operating equipment acc. to EN60079-11 sec: 5.7 in explosive areas Zone 1 und 2.

Contact element: KE ## M ## 0B4H2

Allowed temperatures:

- The maximum surface temperature 95 °C was determined under the following conditions without dust accumulation and safety factor.
- Allowed ambient temperature: -20°C to +60°C.
- Allowed medium temperature in the differential measurement unit < 85°C.



WARNING

Compression heat

With gaseous mediums, the instrument temperature can increase due to compression heat. In such cases, the pressure change speed must be limited or reduced to the allow measuring substance temperature.

NOTICE! For a differential pressure change between 10% and 90% of the measuring range and a pulse frequency < 0.06 Hz, the temperature increase is <10K.

To avoid additional heating, the instruments may not be exposed to direct sunlight during operation.

The standards EN60079-0, EN ISO 80079-36 and EN ISO 80079-37 apply for the non-electrical part of the devices in terms of explosion protection. The applicable requirements of these standards are satisfied.

As a simple electrical operating unit, the installed electrical switch contacts fulfil the requirements of the standard EN60079-14 Par. 3.5.2. The devices are not labelled with respect to the electrical part.

(a) European market (CE):

The documentation for the mechanical part were filed with the notified body NB 0044 TÜV-Nord-Cert under file number 8000324431.

(b) UK market (UKCA):

The documentation for the mechanical part were filed with the notified body NB 2812 Element Material Technology under file number 2812-013.

(c) Eurasian Economic Union (EAC):

The unit does not have ATEX approval for this market. It may only be used there as an industrial unit.

Intrinsically safe power circuits

For use in areas at risk of explosion, instruments must be connected to certified, intrinsically safe electricity circuits.

Max. voltage	U_{\max}	30V
Max. current	I_{\max}	200 mA
Max. power	P_{\max}	800 mW
Max. inner capacity	$C_{i \max}$	60 pF
Max. inner inductivity	$L_{i \max}$	4 µH

Recommend circuit breakers see accessories

3.4.3 Differential pressure transmitter with inductive contacts

DA03 ... 1C

Ex II 2G Ex h IIC T4 Gb

Ex II 2D Ex h IIIC T95°C Db

Explosive areas Zone 1 and 2, and 21 and 22, risk from gases and dry dust.

Contact element: KE ## I ## 0C0H2

Allowed temperatures:

- The maximum surface temperature 95 °C was determined under the following conditions without dust accumulation and safety factor.
- Allowed ambient temperature: -20°C to +60°C.
- Allowed medium temperature in the differential measurement unit < 85°C.



WARNING

Compression heat

With gaseous mediums, the instrument temperature can increase due to compression heat. In such cases, the pressure change speed must be limited or reduced to the allow measuring substance temperature.

NOTICE! For a differential pressure change between 10% and 90% of the measuring range and a pulse frequency < 0.06 Hz, the temperature increase is <10K.

To avoid additional heating, the instruments may not be exposed to direct sunlight during operation.

The standards EN60079-0, EN 60079-31, EN ISO 80079-36 and EN ISO 80079-37 apply for the non-electrical part of the devices in terms of explosion protection. The applicable requirements of these standards are satisfied.

The installed inductive proximity switches of the type SJ2-N (106575) are EC type-tested with the certificate PTB 99 ATEX 2219 X. The type of the installed proximity switch is stated on the type plate. The manufacturer is Pepperl+Fuchs GmbH. For more information about proximity switches, please visit the website <https://www.pepperl-fuchs.com>.

(a) European market (CE):

The documentation for the mechanical part were filed with the notified body NB 0044 TÜV-Nord-Cert under file number 8000324431.

(b) UK market (UKCA):

The documentation for the mechanical part were filed with the notified body NB 2812 Element Material Technology under file number 2812-013.

(c) Eurasian Economic Union (EAC):

The unit does not have ATEX approval for this market. It may only be used there as an industrial unit.

Intrinsically safe power circuits

For use in areas at risk of explosion, instruments must be connected to certified, intrinsically safe electricity circuits.

Max. voltage	U_{\max}	16V
Max. current	I_{\max}	25 mA
Max. power	P_{\max}	64 mW
Max. inner capacity	$C_{i \max}$	30 nF
Max. inner inductivity	$L_{i \max}$	100 µH

Recommend circuit breakers see accessories

3.4.4 Differential pressure transmitter with rotation angle transducer

DA03 ... 2D

II 2G Ex h IIC T4 Gb

Explosive areas Zone 1 and 2, risk from gases.

Rotation angle transducer: KE0905#9

Allowed temperatures:

- The maximum surface temperature 95 °C was determined under the following conditions without dust accumulation and safety factor.
- Allowed ambient temperature: -20°C to +60°C.
- Allowed medium temperature in the differential measurement unit < 85°C.



WARNING

Compression heat

With gaseous mediums, the instrument temperature can increase due to compression heat. In such cases, the pressure change speed must be limited or reduced to the allow measuring substance temperature.

NOTICE! For a differential pressure change between 10% and 90% of the measuring range and a pulse frequency < 0.06 Hz, the temperature increase is <10K.

To avoid additional heating, the instruments may not be exposed to direct sunlight during operation.

The standards EN60079-0, EN ISO 80079-36 and EN ISO 80079-37 apply for the non-electrical part of the devices in terms of explosion protection. The applicable requirements of these standards are satisfied.

The installed capacitive rotation angle measuring transducer of the type KINAX 3W2 are EC type-tested with the certificate ZELM 10 ATEX 0427 X. The type of the installed rotation angle transducer is stated on the type plate. The manufacturer is Camille Bauer Metrawatt AG. For more information about the rotation angle transducer, please visit the website <http://www.camillebauer.com>.

(a) European market (CE):

The documentation for the mechanical part were filed with the notified body NB 0044 TÜV-Nord-Cert under file number 8000324431.

(b) UK market (UKCA):

The documentation for the mechanical part were filed with the notified body NB 2812 Element Material Technology under file number 2812-013.

(c) Eurasian Economic Union (EAC):

The unit does not have ATEX approval for this market. It may only be used there as an industrial unit.

Intrinsically safe power circuits

For use in areas at risk of explosion, instruments must be connected to certified, intrinsically safe electricity circuits.

Max. voltage	U_{\max}	30V
Max. current	I_{\max}	160 mA
Max. power	P_{\max}	1 mW
Max. inner capacity	$C_{i \max}$	10 nF
Max. inner inductivity	$L_{i \max}$	0 µH

Recommend circuit breakers see accessories

4 Commissioning

4.1 General

All electrical supply, operating and measuring lines, and the pressure connections must have been correctly installed before commissioning. All supply lines are arranged so that there are no mechanical forces acting on the device.

Check that all pressure connections are free of leaks before commissioning.

In models filled with fluid, the venting valve on the upper side of the bayonet casing must be opened before commissioning! To do this, turn the venting screw anticlockwise as far as it will go.

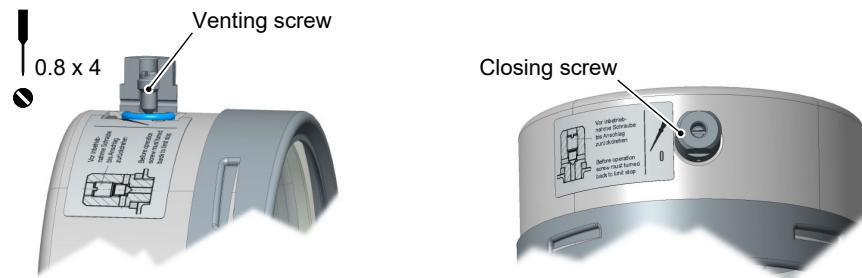


Fig. 14: Venting valve

4.2 Venting of the pressure lines



WARNING

Risk connected to pressure

Never remove the venting screw if the unit is still pressurised! Close the shut-off valves of the flanged fittings or depressurize the system.

The pressure lines need to be vented for before commissioning on devices that work with fluid media. Proceed as follows:

- Remove the venting screws of the two pressure chambers.
- Carefully increase the system pressure until the fluid level is 5 mm below the sealing surface of the threaded borehole.
- Close the device with the venting screws

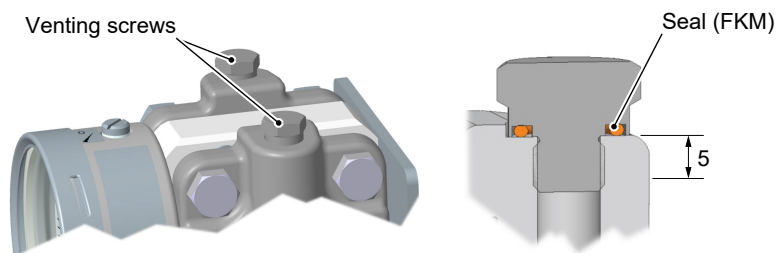


Fig. 15: Venting with fluid media

4.3 Zero point correction

The differential pressure measuring units are set in the factory before delivery so that they do not usually need to be adjusted at the assembly site. If this is still necessary, proceed as follows:

- Depressurize the measuring chamber (+) and (-) side or only exert the existing static system pressure.
- Remove the closing screw The zero point correction screw is located behind.
- Set the measurement value pointer to the scale zero point using the zero point correction screw.
- Mount the closing screw

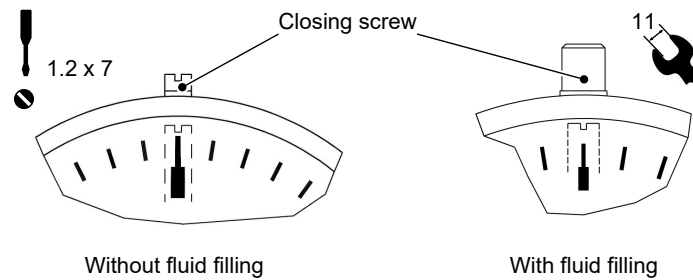


Fig. 16: Zero point correction screw

4.4 Switch point setting

There is an adjustment lock attached to the front pane of the measuring unit on units with contact elements. This means that the contacts attached to the target indicators can be set to any point along the scale.

To facilitate switching precision and the service life of the mechanical measuring system, the switching points should lie between 10% and 90% of the measuring range.

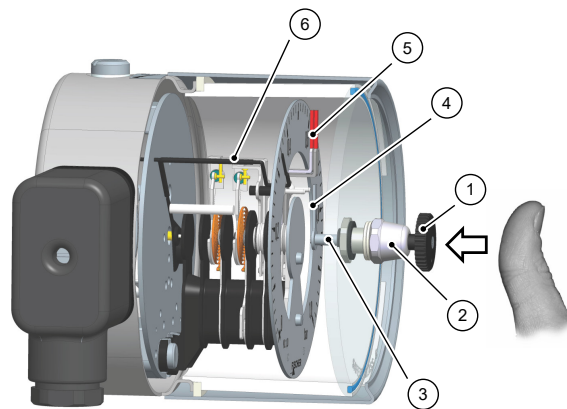


Fig. 17: Switch point setting

1	Adjustment key	2	Adjusting lock
3	Axle	4	Drive arm
5	Set-point display	6	Actual value display

Adjustment sequence:

- Press the axle inwards until the drive arm reaches behind the setting pin of the target value indicator.
- Set the target value indicator to the required switch point by turning the setting key.
- Relieve the axle.
- The switch-point setting can be secured against unintentional adjustment by removing the attachment screw and the adjustment key.

5 Servicing

5.1 Maintenance

The instrument is maintenance-free. We recommend the following regular inspection to guarantee reliable operation and a long service life:

- Check the function in combination with downstream components.
- Check the leak-tightness of the pressure connection lines.
- Check the electrical connections.

The exact test cycles need to be adapted to the operating and environmental conditions. In combination with other devices, the operating instructions for the other devices also need to be observed.

5.2 Maintenance

To ensure reliable operation and a long service life, we recommend carrying out the following test on a regular basis:

- Check the reading.
- Checking the switch function in connection with the downstream components.
- Checking the differential pressure lines for leaks.
- Checking the electrical connections (terminal connection of the cable).

The precise test cycles and operating and ambient conditions need to be adjusted. If several components of the unit interact, all operating instructions of the other units also need to be observed.



WARNING

Dust deposits

The device must be cleaned with a damp cloth at regular intervals to prevent heat build-up. Cleaning intervals depend on the amount of local dust.

5.3 Transport

The measuring device must be protected against impacts. It should be transported in the original packaging or a suitable transport container.

5.4 Service

All defective or faulty devices should be sent directly to our repair department. Please coordinate all shipments with our sales department.



WARNING

Process media residues

Process media residues in and on dismantled devices can be a hazard to people, animals and the environment. Take adequate preventive measures. If required, the devices must be cleaned thoroughly.

Return the device in the original packaging or a suitable transport container.

5.5 Disposal

WEEE-Reg.-No. DE 31751293



Please help to protect our environment and dispose of the workpieces and packaging materials used in an environmentally friendly manner. Observe the country-specific waste treatment and disposal regulations.

The year of production can be found in the production number (serial number):

P# 23 03618.03.123

Production year 2023 —↑

Further information on disposal can be found on our website
[www.fischermesstechnik.de]

6 Technical data

6.1 General information

EXECUTION	Nominal pressure	Measuring cell	Application information
DA03 G ...	PN40	Ø75	Measuring ranges: 0...0.6 bar to 0...25 bar Remote seals: ⁽¹⁾ It is possible to attach remote seals for measuring ranges ≥ 0.6 bar.
DA03 K ...	PN100	Ø75	Measuring ranges: 0...0.6 bar to 0...25 bar Remote seals: It is possible to attach remote seals for measuring ranges ≥ 0.6 bar.
DA03 H ...	PN40	Ø130	Measuring ranges: 0...40 mbar to 0...400 bar Limitations: Drag indicator measuring ranges ≥ 60 mbar Contacts / Transmitter measuring ranges ≥ 100 mbar Remote seals: It is possible to attach remote seals for measuring ranges ≥ 160 mbar..
DA03 L ...	PN100	Ø130	Measuring ranges: 0...40 mbar to 0...400 bar Limitations: Drag indicator measuring ranges ≥ 60 mbar Contacts / Transmitter measuring ranges ≥ 100 mbar Remote seals: It is possible to attach remote seals for measuring ranges ≥ 160 mbar..
DA03 P ...	PN160	Ø130	Measuring ranges: 0...40 mbar to 0...400 bar Limitations: Drag indicator measuring ranges ≥ 60 mbar Contacts / Transmitter measuring ranges ≥ 100 mbar Remote seals: It is possible to attach remote seals for measuring ranges ≥ 0.6 bar.

⁽¹⁾ The remote seals need to be designed for the displacement volume, the length of the cable and the application temperature

6.2 Input variables

Measuring variable

Differential pressure in gaseous and fluid aggressive media.

General information

Rated pressure of the measuring system	Max. static operating pressure
Durability	One-sided over-pressure-proof up to the rated pressure of the measuring system resistance to under-pressure on the (+) and (-) side
Measurement accuracy	±1.6 % of the measuring range
Temperature sensor	0.3 % / 10 °C
Zero-point adjustment	±25 % of the measuring range

Measuring ranges

Small measuring cell Ø75

Measurement range	Device model	
	H	K
0 ... 250 mbar		
0 ... 400 mbar		
-100 ... 150 mbar		
-150 ... 250 mbar		
0...0.6 bar	•	•
0...1 bar	•	•
0...1.6 bar	•	•
0 ... 2.5bar	•	•
0...4.0 bar	•	•
0...6 bar	•	•
0...10 bar	•	•
0...16 bar	•	•
0...25 bar	•	•
-1...0.6 bar	•	•
-1...1.5 bar	•	•
-1...3 bar	•	•
-1...5 bar	•	•

Large measuring cell Ø130

Measurement range	Device model		
	H	L	P
0 ... 40 mbar	•	•	•
0 ... 60 mbar	•	•	•
0 ... 100 mbar	•	•	•
0 ... 160 mbar	•	•	•
0 ... 250 mbar	•	•	•
0 ... 400 mbar	•	•	•
-40 ... +60 mbar	•	•	•
-60 ... +100 mbar	•	•	•
-100 ... +150 mbar	•	•	•
-100 ... +250 mbar	•	•	•

6.3 Operating conditions

Permissible ambient temperature	-20 ... +60 °C
Admissible storage temperature	-40 ... +80 °C
Admissible media temperature	Max. 100 °C
Type of protection:	IP 65 acc. to EN 60529

6.4 Construction design

Materials

Measured value display	Material	Material no.	
		EU	AISI
Bayonet ring housing NG100, NG160	CrNi steel	1.4301	304
Process connection (all models)	CrNi steel	1.4404	316L
Intermediate plate	AlMgSiPb	HARD-COAT®	
Seals	FKM		
Motion train	CrNi steel		
Dial face and needle	Aluminium, painted, printed		
Inspection disk	Safety laminated glass		

MB = Measurement range

Materials (media-contacting)

Design of the measuring system (R)		Material	Material no.	
			EU	AISI
Pressure caps		CrNi steel	1.4404	316L
Measuring membranes	MB ≤ 400 mbar	CrNi steel	1.4571	361Ti
	MB ≥ 0.6 bar	NiCrCo alloy	DURATHERM®	

Design of the measuring system (H)		Material
Pressure caps		Hastelloy® C276
Measuring membranes	MB ≤ 2.5 bar	Hastelloy® C276
	MB ≥ 4 bar	Standard membrane with separator film Hastelloy® C276 The model with the separator foil is not suitable for under-pressure

Design of the measuring system (G)		Material	Material no.	
			EU	AISI
Pressure caps		CrNi steel	1.4404	316L
Measuring membranes	MB ≤ 400 mbar	CrNi steel	1.4571	361Ti
	MB ≥ 0.6 bar	NiCrCo alloy	DURATHERM®	

Process connection	Material	Material no.	
		EU	AISI
Connecting piece and port	CrNi steel	1.4404	316L
Cutting ring screw connections	CrNi steel	1.4571	

Assembly

Wall mounting	Flanged assembly plate
Pipe mounting	Flanged assembly plate and attachment bracket
Panel mounting set type 1	Panel installation fittings for units with a small measuring cell (Ø75) and NG100 bayonet ring casing.
Panel mounting set type 2	Front ring and support construction

6.4.1 Additional Attachments

6.4.1.1 Contact elements

Limit signal transmitters (contacts) and capacitive rotation angle transducers with an output signal proportional to the angular position can be fitted into a housing augmented by a corresponding bayonet ring connector.

A certain minimum pressure level is required to operate this kind of contact element, which is why there is a lower limit for the mbar measuring ranges. This limit depends on the model type and is stated in the section 'General'.

The measuring deviation increases by $\pm 0.5\%$ per contact when the contacts are driven and switched.

For more information and the order key, please refer to the data sheet:

- for limit switch in data sheet KE
- for rotation angle converter in the data sheet KE09

6.4.1.2 Fluid charging

Under aggravated operating conditions, such as vibrations and extreme pressure fluctuations, or in order to avoid condensation forming if used outdoors, the casing can be filled with the following fluids depending in the type of contacts installed:

without contacts	Paraffin oil, Glycerine, silicon oil
Magnetic spring contacts	Silicon oil
Inductive contacts	Paraffin oil, Silicon oil
Rotation angle transducer	no filling possible

6.4.1.3 Marker needle

A settable red marker can be attached to the scale to clearly show a certain pressure (limit value).

6.4.1.4 Trailing needle

The trailing needle is 'dragged' with the measured value indicator. As there is no fixed connection between the two needles, one-off maximum values are stored. The trailing needle can be reset using an adjusting dial in the window. Trailing needles cannot be used in conjunction with contacts. A certain minimum pressure level is required to move the drag indicator, which is why there is a lower limit for the mbar measuring ranges. This limit depends on the model type and is stated in the section 'General [► 26]'.

6.4.1.5 Shut-off fitting

3-spindle valve block PN 420, DN 5, can be directly flanged

- Type DZ3600SV2700
- Material 1.4571
- Functions: Shut-off, pressure compensation

6.4.2 Electrical connection

In the case of devices with auxiliary electronic equipment, the connection is completed using a cable socket attached to the side. The pin assignment depends on the ordered model and is stated in the data sheet KE or KE09.



Cable socket

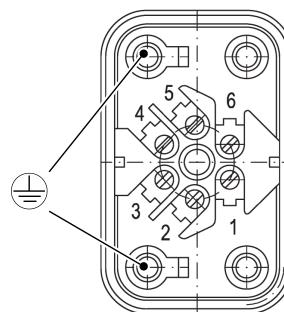


Fig. 18: Cable socket (blue)


Cable socket

Number of screw terminals	6 + 2PE
Rated current	See data sheet KE
Rated voltage	250 V
Conductor cross-section	up to 1.5 mm ² with wire protection
Cable gland	M20 x 1.5
Terminal range	7 ... 13 mm
Tightening torque	3 Nm
Key width	21
Protection class acc. to IEC 529	IP65 (when screwed in)


6.4.3 Dimensional drawings

All dimensions in mm unless otherwise stated

Small measuring system (Ø75)

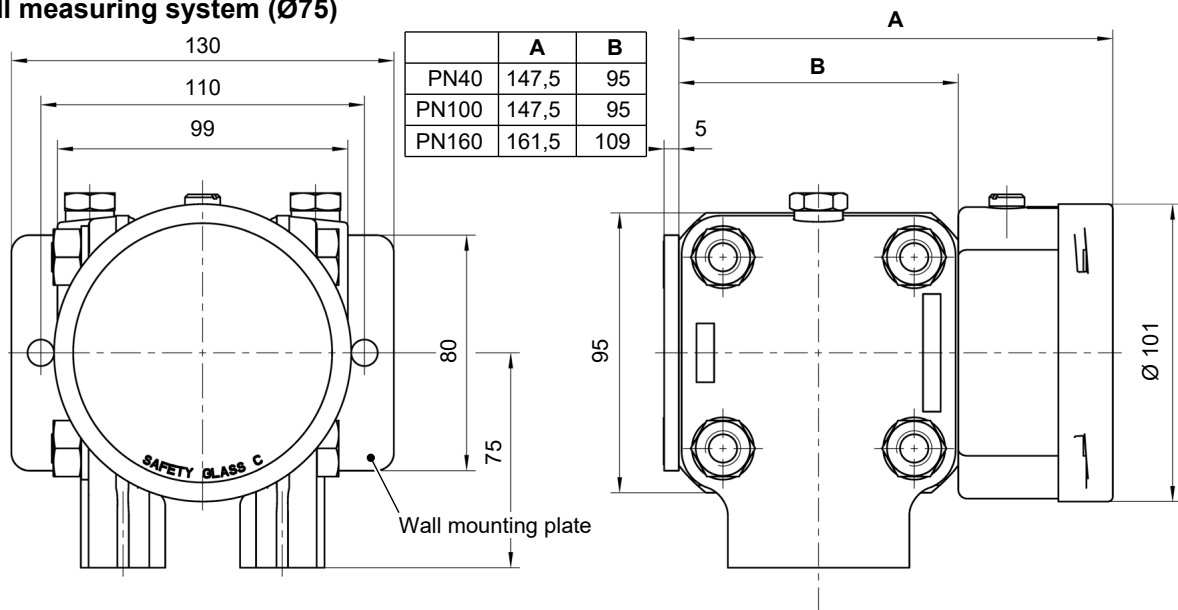

Flange based on DIN EN 61518

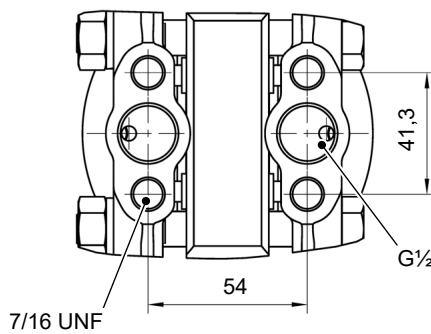

Wall mounting plate

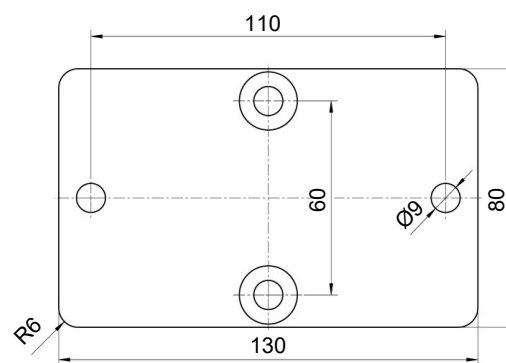


Fig. 19: Dimensional drawing (Small measuring system Ø75)

2" pipe mounting

(possible for all models)

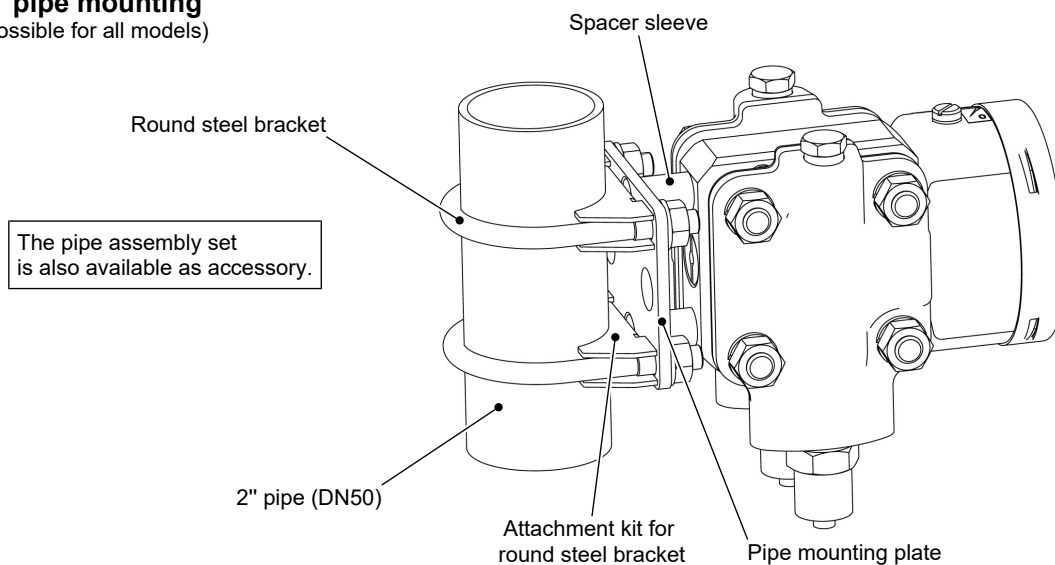


Fig. 20: Pipe mounting





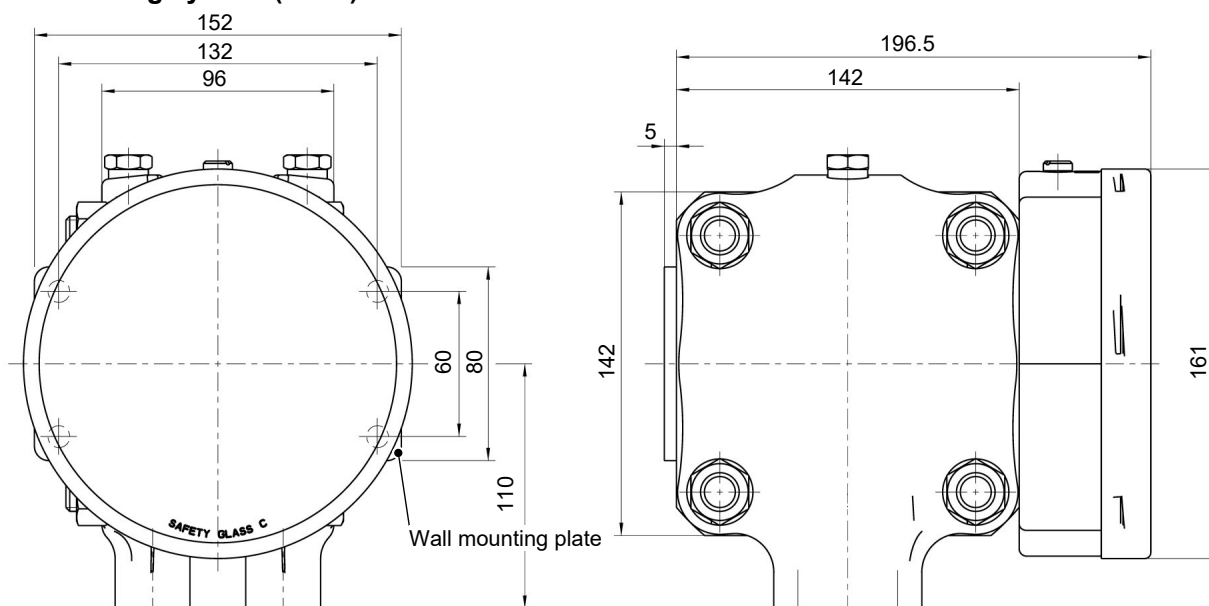
Large measuring system (Ø130)**Flange based on DIN EN 61518****Wall mounting plate**

Fig. 21: Dimensional drawing (Large measuring system Ø130)

Installation of front panel type 1

(only small measuring system Ø75 and NG100 display)

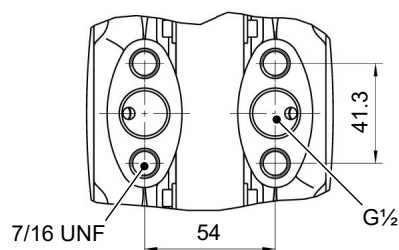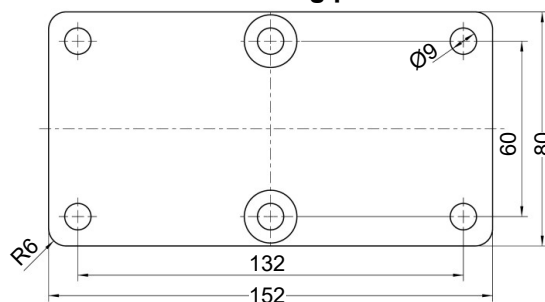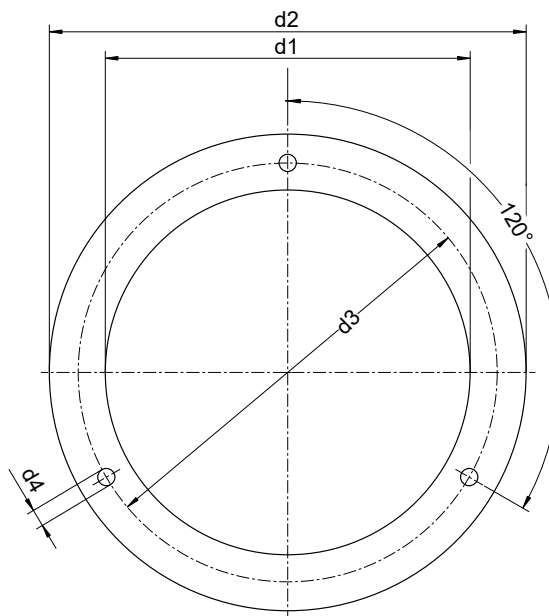
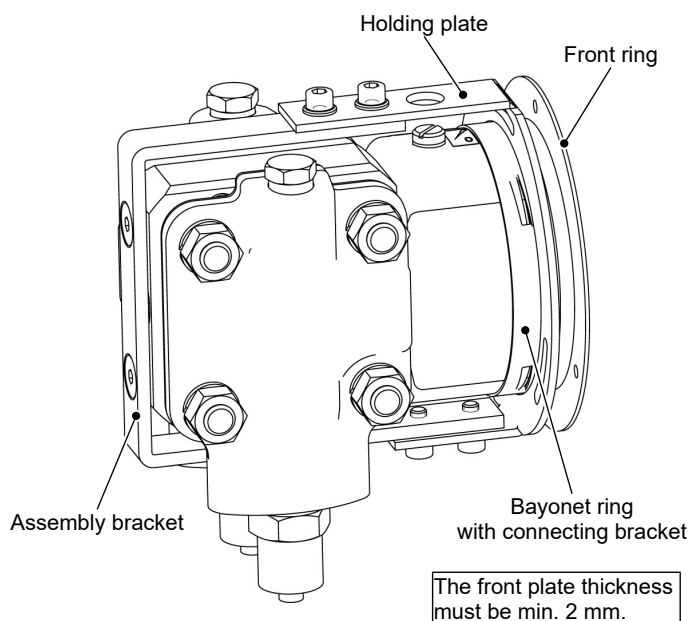


	d1	d2	d3	d4
NG100	101	132	116	4.8

Fig. 22: Installation of front panel with panel fittings

Installation of front panel type 2


The front plate thickness must be min. 2 mm.

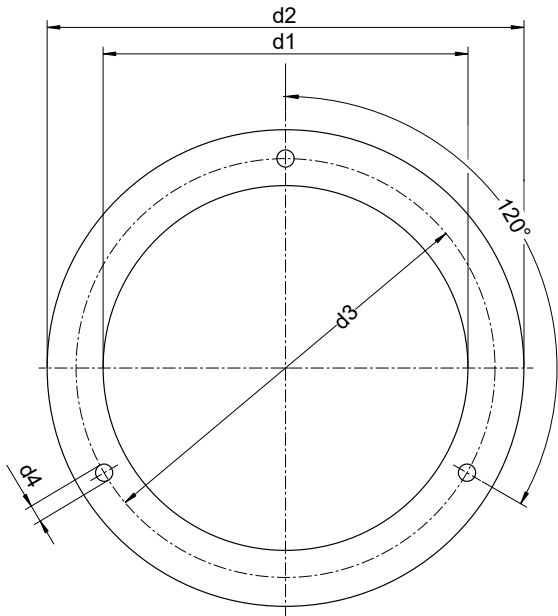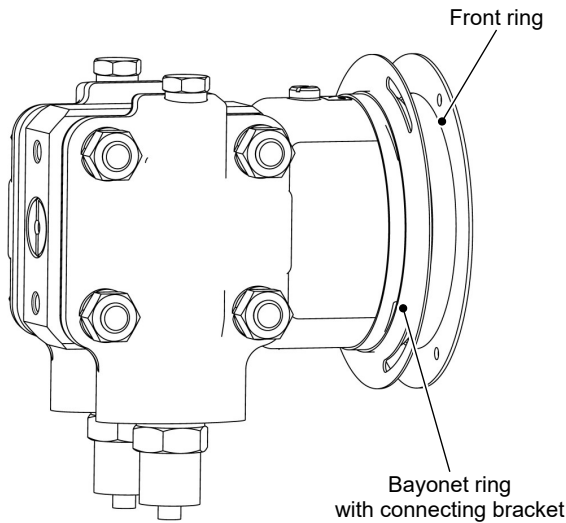


	d1	d2	d3	d4
NG100	101	132	116	4.8
NG160	161	196	178	5.8

A suitable steel construction must be used to ensure that the front plate can bear the weight of the device.

Examples:

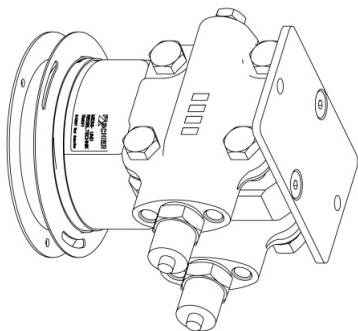

Assembly on a mounting plate

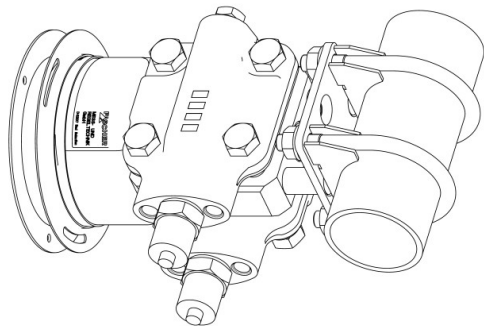

Mounting to a 2" pipe

Fig. 23: Installation of front panel with front ring

Contact elements


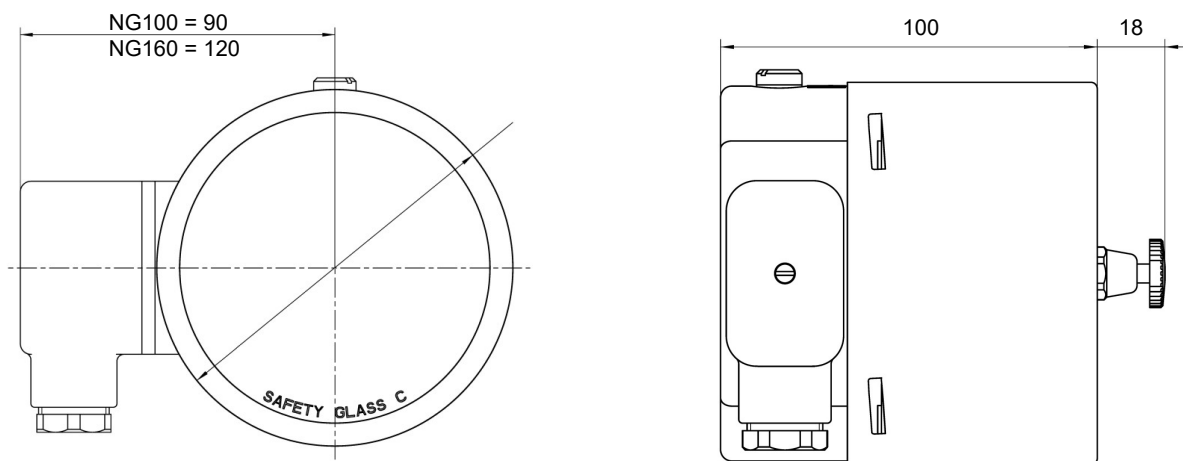


Fig. 24: Dimensional drawing contact devices

Shut-off fitting

with inner spindle thread

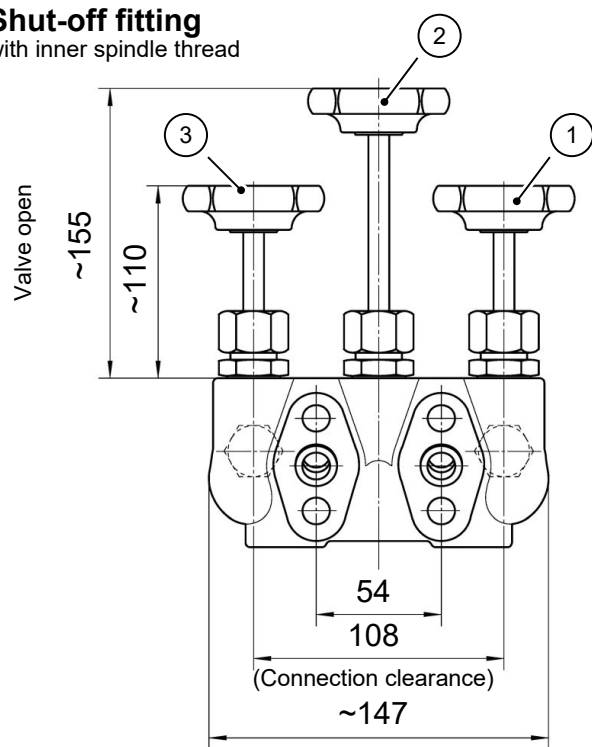

Cutting ring connection G3/8
for 12 mm pipe



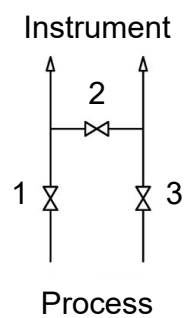


Fig. 25: Shutoff valve DZ3600SV2700

7 Order Codes

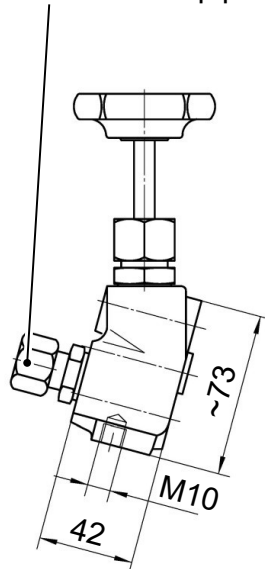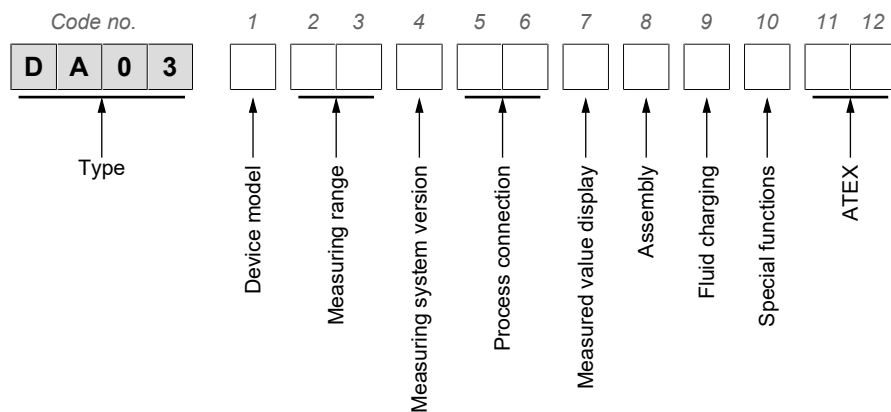

Device model:

[1]	Pressure level	Measuring cell
G	PN40	Ø75
H	PN40	Ø130
K	PN100	Ø75
L	PN100	Ø130
P	PN160	Ø130

Measuring range:

Small measuring system
Ø75

[2.3]	Measurement range	Device model	
		G	K
82	0 ... 250 mbar		
83	0 ... 400 mbar		
74	-100 ... 150 mbar		
76	-150 ... 250 mbar		
01	0...0.6 bar	•	•
02	0...1 bar	•	•
03	0...1.6 bar	•	•
04	0 ... 2.5bar	•	•
05	0...4.0 bar	•	•
06	0...6 bar	•	•
07	0...10 bar	•	•
08	0...16 bar	•	•
09	0...25 bar	•	•
32	-1...0.6 bar	•	•
33	-1...1.5 bar	•	•
34	-1...3 bar	•	•
35	-1...5 bar	•	•

**Large measuring system
Ø130**

[2.3]	Measurement range	Device model		
		H	L	P
57	0 ... 40 mbar	•	•	•
58	0 ... 60 mbar	•	•	•
59	0 ... 100 mbar	•	•	•
60	0 ... 160 mbar	•	•	•
82	0 ... 250 mbar	•	•	•
83	0 ... 400 mbar	•	•	•
70	-40 ... +60 mbar	•	•	•
72	-60 ... +100 mbar	•	•	•
74	-100 ... +150 mbar	•	•	•
76	-100 ... +250 mbar	•	•	•

Design of the measuring system:

[4]	
R	Pressure chamber CrNi steel 1.4404 (AISI 316L) Measuring membrane standard
H	Pressure chamber Hastelloy C4 Measuring membrane Hastelloy C276
G	Pressure chamber CrNi steel 1.4404 (AISI 316L) Measuring membrane Hastelloy C276

Process connection:

[5.6]	
03	Flange connection based on DIN EN 61518 with internal thread G $\frac{1}{2}$
04	Connecting piece G $\frac{1}{2}$ with inside thread 1/4 -18 NPT
05	Connecting piece G $\frac{1}{2}$ with inside thread 1/2 -14 NPT
13	Connection shanks G $\frac{1}{2}$ with external thread G $\frac{1}{2}$
14	Connecting port G $\frac{1}{2}$ with outer thread 1/4-18 NPT
15	Connecting port G $\frac{1}{2}$ with outer thread 1/2-14 NPT
27	Cutting ring connection in brass for 12 mm pipe

Measured value display:

[7]	
L	Bayonet ring housing NG100
M	Bayonet ring housing NG160

Assembly:

[8]	
W	Wall mounting
R	Pipe mounting
T	Panel installation fittings (only a small measuring system Ø75, NG100 measured value display without contact elements)
G	Front ring for panel mounting

Fluid filling:

[9]	
0	Without fluid filling
1	Glycerine
4	Paraffin oil
5	Silicon oil

Special functions:

[10]	
0	Without special function
1	Adjustable marker needle
2	Resettable drag needle

Contacts/transmitters/ATEX:

[11.12] ATEX model		
0A	Non-electrical unit (without switch contacts)	II 2G Ex h IIC T4 Gb II 2D Ex h IIIC T95°C Db
1B	Unit with snap-action contacts KE##M##0B4H2 Simple electrical operating equipment acc. to DIN EN 60079-11	II 2G Ex h IIC T4 Gb
1C	Unit with inductive contacts KE##I##0C0H2	II 2G Ex h IIC T4 Gb II 2D Ex h IIIC T95°C Db
2D	Unit with capacitive rotation angle transducer KE0905#9	II 2G Ex h IIC T4 Gb

Limitations

A minimum operating pressure, which not all measuring ranges achieve, is required to activate a contact element or a drag indicator. Please also note the information about the equipment features [► 10].

7.1 Accessories

Order no.	Planned measures	Material
DZ3600SV2700	Triple valve block DN5 PN420 <ul style="list-style-type: none"> • Flange connection acc. to DIN EN 61518 • Cutting ring screw connections 12 mm pipe • Including assembly set 	1.4571
Order no.	Designation	Type
05003090	Galvanically isolated supply isolating amplifier for ATEX applications. <ul style="list-style-type: none"> • 24 V DC, 1 channel Input: 4 ... 20 mA Output: 4 ... 20 mA • The device can be mounted in Zone 2 / Cl.1, Div. 2 and can receive signals from Zones 0, 1 and 2, as well as 20, 21 and 22 including Mining / Class I/II/III, Div. 1, Size A-G. • SIL2/SIL3 according to IEC 61508 	9106B1A
05003091	Pulse isolator for the transmission of signals from NAMUR sensors and mechanical switches from the ATEX area to the safe area. <ul style="list-style-type: none"> • 24 V DC, 1 channel Switching input (NAMUR) Relay output • The device can be used in safe areas and in zone 2 / div. 2 and can accept signals from zone 0, 1, 2, 20, 21, 22 as well as M1 / class I/II/III, div. 1, size A-G. • SIL2 according to IEC 61508 	9202B2A
05003092	Pulse isolator for the transmission of signals from NAMUR sensors and mechanical switches from the ATEX area to the safe area. <ul style="list-style-type: none"> • 24 V DC, 2 channel Switching input(NAMUR) Relay output • The device can be used in safe areas and in zone 2 / div. 2 and can accept signals from zone 0, 1, 2, 20, 21, 22 as well as M1 / class I/II/III, div. 1, size A-G. • SIL2 according to IEC 61508 	9202B2B
05003093	Display / Programming front Communication interface for setting the operating parameters for supply isolating amplifiers and pulse isolators. <ul style="list-style-type: none"> • The device may only be used in safe areas. • Allows saving the configuration of a device type and loading it into other devices of the same type. • Display for process data and status visualization. 	4501

8 EU Declaration of Conformity



(Translation) **CE**

EU Declaration of Conformity

For the product described as follows

Product designation **Differential Pressure Gauge**
(without contact device)

Type designation **DA03 ... 0A**

it is hereby declared that it corresponds with the basic requirements
specified in the following designated directives:

2014/34/EU

ATEX Directive

2011/65/EU

RoHS Directive

(EU) 2015/863

Delegated Directive amending Annex II to Directive 2011/65/EU

The products were tested in compliance with the following standards.

Explosive atmospheres (ATEX)

DIN EN IEC 60079-0:2019-09

Explosive atmospheres - Part 0: Equipment - General requirements

EN IEC 60079-0:2018

Correction 1

IEC 60079-0:2017/COR1:2020

Explosive atmospheres - Part 31: Equipment dust ignition protection by enclosure "t"

DIN EN 60079-31:2014-12

EN 60079-31:2014

DIN EN ISO 80079-36:2016-12

Explosive atmospheres - Part 36: Non-electrical equipment for explosive atmospheres - Basic method and requirements

EN ISO 80079-36:2016

DIN EN ISO 80079-37:2016-12

Explosive atmospheres - Part 37: Non-electrical equipment for explosive atmospheres - Non-electrical type of protection constructional safety "c", control of ignition sources "b", liquid immersion "k"

EN ISO 80079-37:2016

RoHS Directive (RoHS 3)

DIN EN IEC 63000:2019-05

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

EN IEC 63000:2018

The dossier is retained under file no. **8000324431** at the notified body **NB0044** :

TÜV NORD CERT GmbH

Langemarckstraße 20

45141 Essen

Also they were subjected to the conformity assessment procedure „Internal production control“.

Sole responsibility for the issue of this declaration of conformity in relation to fulfilment of the fundamental requirements and the production of the technical documents is with the manufacturer.

Manufacturer

FISCHER Mess- und Regeltechnik GmbH

Bielefelder Str. 37a

32107 Bad Salzufen, Germany

Tel. +49 (0)5222 974 0

The devices bear the following marking:

CE II 2G Ex h IIC T4 Gb
 II 2D Ex h IIIC T95°C Db

Bad Salzufen
03 Mar 2025

T. Malischewski
Managing Director

09010185 • CE EN DA03_0A • Rev. ST4-B • 03/25

1 / 1



Fig. 26: CE_DE_DA03...0A

(Translation) **CE**

EU Declaration of Conformity

For the product described as follows

Product designation

Differential Pressure Gauge
(with snap action contacts KE ## M ## 0B4H2)

Type designation

DA03 ... 1B

it is hereby declared that it corresponds with the basic requirements specified in the following designated directives:

2014/35/EU
2014/34/EU
2011/65/EU
(EU) 2015/863

Low Voltage Directive
ATEX Directive
RoHS Directive
Delegated Directive amending Annex II to Directive 2011/65/EU

The products were tested in compliance with the following standards.

Low Voltage Directive (LVD)

DIN EN 61010-1:2020-03
EN 61010-1:2010 + A1:2019 + A1:2019/
AC:2019

Safety requirements for electrical equipment for measurement, control, and laboratory use -
Part 1: General requirements

Explosive atmospheres (ATEX)

DIN EN IEC 60079-0:2019-09
EN IEC 60079-0:2018
Correction1
IEC 60079-0:2017/COR1:2020

Explosive atmospheres - Part 0: Equipment - General requirements

DIN EN ISO 80079-36:2016-12
EN ISO 80079-36:2016

Explosive atmospheres - Part 36: Non-electrical equipment for explosive atmospheres - Basic method and requirements

DIN EN ISO 80079-37:2016-12
EN ISO 80079-37:2016

Explosive atmospheres - Part 37: Non-electrical equipment for explosive atmospheres - Non-electrical type of protection constructional safety "c", control of ignition sources "b", liquid immersion "k"

The build-in contact device as an 'standard electrical equipment' meets the requirements of paragraph 3.5.2 of the following standard

DIN EN 60079-14:2014-10
EN 60079-14:2014

Explosive atmospheres - Part 14: Electrical installations design, selection and erection

DIN EN 60079-14 Corrigendum 1:2016-06
EN 60079-14:2014/AC:2016

Corrigendum to DIN EN 60079-14

RoHS Richtlinie (RoHS 3)

DIN EN IEC 63000:2019-05
EN IEC 63000:2018

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

The dossier is retained under file no. **8000324431** at the notified body **NB0044** :

TÜV NORD CERT GmbH
Langemarckstraße 20

45141 Essen

Also they were subjected to the conformity assessment procedure „Internal production control“.

Sole responsibility for the issue of this declaration of conformity in relation to fulfilment of the fundamental requirements and the production of the technical documents is with the manufacturer.

09010186 • CE_EN_DA03_1B • Rev. ST4-B • 03/25



1 / 2

Fig. 27: CE_DE_DA03...1B_Page_01

Manufacturer**FISCHER Mess- und Regeltechnik GmbH**Bielefelder Str. 37a
32107 Bad Salzuflen, Germany
Tel. +49 (0)5222 974 0**The devices bear the
following marking:****CE**  II 2G Ex h IIC T4 Gb**Bad Salzuflen
03 Mar 2025**

T. Malischewski
Managing Director



(Translation)

EU Declaration of Conformity

For the product described as follows

Product designation **Differential Pressure Gauge**
(with inductive contacts KE ## I ## 0C0H2)

Type designation **DA03 ... 1C**

it is hereby declared that it corresponds with the basic requirements specified in the following designated directives:

2014/34/EU

ATEX Directive

2011/65/EU

RoHS Directive

(EU) 2015/863

Delegated Directive amending Annex II to Directive 2011/65/EU

The products were tested in compliance with the following standards.

Explosive atmospheres (ATEX)

DIN EN IEC 60079-0:2019-09
EN IEC 60079-0:2018

Explosive atmospheres - Part 0: Equipment - General requirements

Correction1

IEC 60079-0:2017/COR1:2020

Explosive atmospheres - Part 31: Equipment dust ignition protection by enclosure "t"

DIN EN 60079-31:2014-12

EN 60079-31:2014

Explosive atmospheres - Part 36: Non-electrical equipment for explosive atmospheres - Basic method and requirements

DIN EN ISO 80079-36:2016-12

EN ISO 80079-36:2016

Explosive atmospheres - Part 37: Non-electrical equipment for explosive atmospheres - Non-electrical type of protection constructional safety "c", control of ignition sources "b", liquid immersion "k"

DIN EN ISO 80079-37:2016-12

EN ISO 80079-37:2016

RoHS Directive (RoHS 3)

DIN EN IEC 63000:2019-05
EN IEC 63000:2018

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

The dossier is retained under file no. **8000324431** at the notified body **NB0044** :

TÜV NORD CERT GmbH

Langemarckstraße 20

45141 Essen

The built-in inductive proximity switches are EC type certified: **PTB 99 ATEX 2219 X**

Also they were subjected to the conformity assessment procedure „**Internal production control**".


Sole responsibility for the issue of this declaration of conformity in relation to fulfilment of the fundamental requirements and the production of the technical documents is with the manufacturer.

Manufacturer **FISCHER Mess- und Regeltechnik GmbH**

Bielefelder Str. 37a
32107 Bad Salzuflen, Germany

Tel. +49 (0)5222 974 0

The devices bear the following marking:



Bad Salzuflen
03 Mar 2025

T. Malischewski
Managing Director

09010187 • CE EN DA03_1C • Rev. ST4-B • 03/25

1 / 1



Fig. 29: CE_DE_DA03...1C

(Translation) **CE**

EU Declaration of Conformity

For the product described as follows

Product designation

Differential Pressure Gauge
(with transmitter for angular position KE0905#9)

Type designation

DA03 ... 2D

it is hereby declared that it corresponds with the basic requirements specified in the following designated directives:

2014/30/EU
2014/34/EU
2011/65/EU
(EU) 2015/863

EMC Directive
ATEX Directive
RoHS Directive
Delegated Directive amending Annex II to Directive 2011/65/EU

The products were tested in compliance with the following standards.

Electromagnetic compatibility (EMC)

DIN EN IEC 61000-6-2:2019-11
EN IEC 61000-6-2:2019
DIN EN 61000-6-3:2022-06
EN IEC 61000-6-3:2021

Electromagnetic compatibility (EMC) - Part 6-2: Generic standards - Immunity standard for industrial environments
Electromagnetic compatibility (EMC) - Part 6-3: Generic standards - Emission standard for equipment in residential environments

Explosive atmospheres (ATEX)

DIN EN IEC 60079-0:2019-09
EN IEC 60079-0:2018
Correction 1
IEC 60079-0:2017/COR1:2020
DIN EN ISO 80079-36:2016-12
EN ISO 80079-36:2016
DIN EN ISO 80079-37:2016-12
EN ISO 80079-37:2016

Explosive atmospheres - Part 0: Equipment - General requirements

Explosive atmospheres - Part 36: Non-electrical equipment for explosive atmospheres - Basic method and requirements

Explosive atmospheres - Part 37: Non-electrical equipment for explosive atmospheres - Non-electrical type of protection constructional safety "c", control of ignition sources "b", liquid immersion "k"

RoHS Directive (RoHS 3)

DIN EN IEC 63000:2019-05
EN IEC 63000:2018

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

The dossier is retained under file no. **8000324431** at the notified body **NB0044** :

TÜV NORD CERT GmbH

Langemarckstraße 20
45141 Essen

The build-in transmitter for angular position is EC type certified: **ZELM 10 ATEX 0427 X**

Also they were subjected to the conformity assessment procedure „Internal production control“.

Sole responsibility for the issue of this declaration of conformity in relation to fulfilment of the fundamental requirements and the production of the technical documents is with the manufacturer.

Manufacturer

FISCHER Mess- und Regeltechnik GmbH

Bielefelder Str. 37a
32107 Bad Salzuflen, Germany
Tel. +49 (0)5222 974 0

The devices bear the following marking:

CE II 2G Ex h IIC T4 Gb

Bad Salzuflen
03 Mar 2025

T. Malischewski
Managing Director

09010188 • CE_EN_DA03_2D • Rev. ST4-A • 01/18



1 / 1

Fig. 30: CE_DE_DA03...2D

9 UKCA Declarations of Conformity



UKCA Declaration of Conformity

For the product described as follows

Product designation **Differential Pressure Gauge**
(without contact device)

Type designation **DA03 ... 0A**

is hereby declared to comply with the essential requirements, specified in the following UK regulations:

Statutory regulation No.	Description
2016 No. 1107	<i>The Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres Regulations 2016</i>
2022 No. 1647	<i>The Hazardous Substances and Packaging (Legislative Functions and Amendment) (EU Exit) Regulations 2020</i>
2021 No. 422	<i>The Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment (Amendment) Regulations 2021</i>

The products have been tested according to the following standards.

Explosive atmospheres (ATEX):

<i>BS EN IEC 60079-0:2018-07-09</i>	<i>Explosive atmospheres. Equipment. General requirements</i>
<i>BS EN 60079-31:2014-07-31</i>	<i>Explosive atmospheres. Equipment dust ignition protection by enclosure "t"</i>
<i>BS EN ISO 80079-36:2016-04-30</i>	<i>Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Basic method and requirements</i>
<i>BS EN ISO 80079-37:2016-04-30</i>	<i>Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Non electrical type of protection constructional safety "c", control of ignition source "b", liquid immersion "k"</i>

Restriction of Hazardous Substances (RoHS):


<i>BS EN IEC 63000:2018-12-10</i>	<i>Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances</i>
-----------------------------------	---

The documents are kept under file number **2812-013** at the notified body **NB-No. 2812**.

Element Materials Technology

Unit 1 Pendle Place
Skelmersdale, WN8 9PN, United Kingdom

The devices bear the following marking:



The sole responsibility for drawing up this declaration of conformity in relation to the fulfilment of the essential requirements and the preparation of the technical documentation lies with the manufacturer.

Manufacturer

FISCHER Mess- und Regeltechnik GmbH

Bielefelder Str. 37a
32107 Bad Salzufflen, Germany
Tel. +49 (0)5222 974 0

Bad Salzufflen
04 Okt 2021

G. Gödde
Managing director

09010588 • UKCA_EN_DA03_0A • Rev. ST4-A • 09/21



1 / 1

Fig. 31: UKCA_EN_DA03_0A



UKCA Declaration of Conformity

For the product described as follows

Product designation **Differential Pressure Gauge**
(with snap action contacts KE ## M ## 0B4H2)

Type designation **DA03 ... 1B**

is hereby declared to comply with the essential requirements, specified in the following UK regulations:

Statutory regulation No.	Description
2016 No. 1107	<i>The Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres Regulations 2016</i>
2016 No. 1101	<i>The Electrical Equipment (Safety) Regulations 2016</i>
2022 No. 1647	<i>The Hazardous Substances and Packaging (Legislative Functions and Amendment) (EU Exit) Regulations 2020</i>
2021 No. 422	<i>The Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment (Amendment) Regulations 2021</i>

The products have been tested according to the following standards.

Explosive atmospheres (ATEX):

<i>BS EN IEC 60079-0:2018-07-09</i>	<i>Explosive atmospheres. Equipment. General requirements</i>
<i>BS EN ISO 80079-36:2016-04-30</i>	<i>Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Basic method and requirements</i>
<i>BS EN ISO 80079-37:2016-04-30</i>	<i>Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Non electrical type of protection constructional safety "c", control of ignition source "b", liquid immersion "k"</i>

The installed electrical switching contacts fulfil the requirements of the following standard as 'simple electrical equipment' according to paragraph 3.5.2.

<i>BS EN 60079-14:2014-06-30</i>	<i>Explosive atmospheres. Electrical installations design, selection and erection.</i>
----------------------------------	--

Low Voltage Directive (LVD):

<i>BS EN 61010-1+A1:2017-03-31</i>	<i>Safety requirements for electrical equipment for measurement, control, and laboratory use. General requirements</i>
------------------------------------	--

Restriction of Hazardous Substances (RoHS):

<i>BS EN IEC 63000:2018-12-10</i>	<i>Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances</i>
-----------------------------------	---

The documents are kept under file number **2812-013** at the notified body **NB-No. 2812**.

Element Materials Technology

Unit 1 Pendle Place
Skelmersdale, WN8 9PN, United Kingdom

The devices bear the following marking:



Fig. 32: UKCA_EN_DA03_1B_Page_1

The sole responsibility for drawing up this declaration of conformity in relation to the fulfilment of the essential requirements and the preparation of the technical documentation lies with the manufacturer.

Manufacturer**FISCHER Mess- und Regeltechnik GmbH**

Bielefelder Str. 37a
32107 Bad Salzuflen, Germany

Tel. +49 (0)5222 974 0



Bad Salzuflen
04 Okt 2021

G. Götde
Managing director



Fig. 33: UKCA_EN_DA03_1B_Page_2



UKCA Declaration of Conformity

For the product described as follows

Product designation **Differential Pressure Gauge**
(with inductive contacts KE ## I ## 0C0H2)

Type designation **DA03 ... 1C**

is hereby declared to comply with the essential requirements, specified in the following UK regulations:

Statutory regulation No.	Description
2016 No. 1107	The Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres Regulations 2016
2016 No. 1091	The Electromagnetic Compatibility Regulations 2016
2022 No. 1647	The Hazardous Substances and Packaging (Legislative Functions and Amendment) (EU Exit) Regulations 2020
2021 No. 422	The Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment (Amendment) Regulations 2021

The products have been tested according to the following standards.

Explosive atmospheres (ATEX):

BS EN IEC 60079-0:2018-07-09	Explosive atmospheres. Equipment. General requirements
BS EN 60079-31:2014-07-31	Explosive atmospheres. Equipment dust ignition protection by enclosure "t"
BS EN ISO 80079-36:2016-04-30	Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Basic method and requirements
BS EN ISO 80079-37:2016-04-30	Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Non electrical type of protection constructional safety "c", control of ignition source "b", liquid immersion "k"

The built-in inductive proximity switches are EC type tested: **PTB 99 ATEX 2219 X**.

Electromagnetic compatibility (EMC):

BS EN IEC 61000-6-2:2019-02-25	Electromagnetic compatibility (EMC). Generic standards. Immunity standard for industrial environments
BS EN IEC 61000-6-3:2021-03-30	Electromagnetic compatibility (EMC). Generic standards. Emission standard for equipment in residential environments

Restriction of Hazardous Substances (RoHS):


BS EN IEC 63000:2018-12-10	Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances
----------------------------	--

The documents are kept under file number **2812-013** at the notified body **NB-No. 2812**.

Element Materials Technology

Unit 1 Pendle Place
Skelmersdale, WN8 9PN, United Kingdom

The devices bear the following marking:



The sole responsibility for drawing up this declaration of conformity in relation to the fulfilment of the essential requirements and the preparation of the technical documentation lies with the manufacturer.

Manufacturer**FISCHER Mess- und Regeltechnik GmbH**

Bielefelder Str. 37a
32107 Bad Salzuflen, Germany

Tel. +49 (0)5222 974 0



Bad Salzuflen
04 Okt 2021

G. Gödde
Managing director





UKCA Declaration of Conformity

For the product described as follows

Product designation **Differential Pressure Gauge**
(with transmitter for angular position KE0905#9)

Type designation **DA03 ... 2D**

is hereby declared to comply with the essential requirements, specified in the following UK regulations:

Statutory regulation No.	Description
2016 No. 1107	<i>The Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres Regulations 2016</i>
2016 No. 1091	<i>The Electromagnetic Compatibility Regulations 2016</i>
2022 No. 1647	<i>The Hazardous Substances and Packaging (Legislative Functions and Amendment) (EU Exit) Regulations 2020</i>
2021 No. 422	<i>The Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment (Amendment) Regulations 2021</i>

The products have been tested according to the following standards.

Explosive atmospheres (ATEX):

<i>BS EN IEC 60079-0:2018-07-09</i>	<i>Explosive atmospheres. Equipment. General requirements</i>
<i>BS EN ISO 80079-36:2016-04-30</i>	<i>Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Basic method and requirements</i>
<i>BS EN ISO 80079-37:2016-04-30</i>	<i>Explosive atmospheres. Non-electrical equipment for explosive atmospheres. Non electrical type of protection constructional safety "c", control of ignition source "b", liquid immersion "k"</i>

The built-in angle of rotation transducer is EC type-tested: **ZELM 10 ATEX 0427 X**.

Electromagnetic compatibility (EMC):

<i>BS EN IEC 61000-6-2:2019-02-25</i>	<i>Electromagnetic compatibility (EMC). Generic standards. Immunity standard for industrial environments</i>
<i>BS EN IEC 61000-6-3:2021-03-30</i>	<i>Electromagnetic compatibility (EMC). Generic standards. Emission standard for equipment in residential environments</i>

Restriction of Hazardous Substances (RoHS):

<i>BS EN IEC 63000:2018-12-10</i>	<i>Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances</i>
-----------------------------------	---

The documents are kept under file number **2812-013** at the notified body **NB-No. 2812**.

Element Materials Technology

Unit 1 Pendle Place
Skelmersdale, WN8 9PN, United Kingdom

The devices bear the following marking:



Ex II 2G Ex h IIC T4 Gb

09010594 • UKCA_EN_DA03_2D • Rev. ST4-A • 09/21



1 / 2

Fig. 36: UKCA_EN_DA03_1C_Page_2

The sole responsibility for drawing up this declaration of conformity in relation to the fulfilment of the essential requirements and the preparation of the technical documentation lies with the manufacturer.

Manufacturer**FISCHER Mess- und Regeltechnik GmbH**

Bielefelder Str. 37a
32107 Bad Salzuflen, Germany

Tel. +49 (0)5222 974 0



Bad Salzuflen
04 Okt 2021

G. Gödde
Managing director



Fig. 37: UKCA_EN_DA03_2D_Page_2

10 EAC Declaration



ЕВРАЗИЙСКИЙ ЭКОНОМИЧЕСКИЙ СОЮЗ ДЕКЛАРАЦИЯ О СООТВЕТСТВИИ

Заявитель Общество с ограниченной ответственностью «МАТИС-М». Место нахождения: 117261, город Москва, улица Вавилова, дом 70, корпус 3, комната правления, Российская Федерация. Адрес места осуществления деятельности: 109029, город Москва, город, Сибирский проезд, дом 2, корпус 12, Российская Федерация, Основной государственный регистрационный номер: 1037739575125, телефон: +7 495 725-23-09, адрес электронной почты: info@matis-m.ru

в лице Генерального директора Шарова Александра Анатольевича

заявляет, что Прибор - манометр для измерения дифференциального давления, тип DA01, DA03, DA08, DA09, DA10, DA12

Продукция изготовлена в соответствии с директивой 2014/30/EU

Изготовитель "FISCHER Mess- und Regeltechnik GmbH"

Место нахождения: Bielefelder StraBe 37a, D-32107 Bad Salzuflen, Германия. Филиал завода-изготовителя: "FISCHER Mess- und Regeltechnik GmbH" место нахождения: Bielefelder StraBe 37a, D-32107 Bad Salzuflen, Германия.

Код ТН ВЭД ЕАЭС 9026 20 400 0, серийный выпуск

Соответствует требованиям Технического регламента Таможенного союза ТР ТС 020/2011 "Электромагнитная совместимость технических средств"

Декларация о соответствии принята на основании протокола № 01228-02/2017-06 от 14.06.2017 года. Испытательной лаборатории (центра) продукции народного потребления "Отдел 101" Общества с ограниченной ответственностью "Межрегиональный центр исследований и испытаний", регистрационный номер аттестата аккредитации № RA.RU.21AO47 Схема декларирования: 3д

Дополнительная информация ГОСТ 30804.3.2-2013 Совместимость технических средств электромагнитная. Эмиссия гармонических составляющих тока техническими средствами с потребляемым током не более 16 А (в одной фазе). Нормы и методы испытаний

ГОСТ 30804.3.3-2013 Совместимость технических средств электромагнитная. Ограничение изменений напряжения, колебаний напряжения и фликера в низковольтных системах электроснабжения общего назначения. Технические средства с потребляемым током не более 16 А (в одной фазе), подключаемые к электрической сети при несоблюдении определенных условий подключения. Нормы и методы испытаний
Условия хранения продукции в соответствии с ГОСТ 15150-69. Срок хранения (службы, годности) указан в прилагаемой к продукции товаросопроводительной и/или эксплуатационной документации.

Декларация о соответствии действительна с даты регистрации по 14.06.2022 включительно


(подпись)

М.П.

Шаров Александр Анатольевич

(Ф. И. О. заявителя)

Регистрационный номер декларации о соответствии: ЕАЭС N RU Д-ДЕ.АЛ16.В.77754

Дата регистрации декларации о соответствии: 15.06.2017

Notes

Notes

Notes



FISCHER Mess- und Regeltechnik GmbH

Bielefelder Str. 37a
D-32107 Bad Salzuflen

Tel. +49 5222 974-0

Fax +49 5222 7170

www.fischermesstechnik.de
info@fischermesstechnik.de